



ORIGINAL ARTICLE/ARTICOLO ORIGINALE

Comparison of shaping ability of ProTaper Next and 2Shape nickel–titanium files in simulated severe curved canals

Analisi sperimentale della preparazione endodontica in canali artificiali con curvature complesse: ProTaper Next Vs. 2Shape

Simone Staffoli^{a,*}, Taha Özyürek^b, Avi Hadad^c, Alex Lvovsky^c, Michael Solomonov^c, Hadas Azizi^c, Joe Ben Itzhak^c, Maurizio Bossù^a, Nicola M. Grande^d, Gianluca Plotino^e, Antonella Polimeni^a

^a Department of Oral & Maxillofacial Science, Sapienza University of Rome, Italy

^b Department of Endodontics, Faculty of Dentistry, Istanbul Medeniyet University, Samsun, Turkey

^c Department of Endodontics, Israel Defense Forces Medical Corps, Tel Hashomer, Israel

^d Department of Endodontics, Catholic University of Sacred Heart, Rome, Italy

^e Private Practice, Grande Plotino & Torsello – Studio di Odontoiatria, Rome, Italy

Received 10 May 2018; accepted 10 May 2018

Available online 13 July 2018

KEYWORDS

Centering ability;
Centering ratio;
Heat treatment;
2Shape;
ProTaper Next.

Abstract

Aim: To evaluate the centering ability of ProTaper Next (PTN) and 2Shape (TS) nickel–titanium (NiTi) instruments in terms of maintaining the original root canal configuration in a simulated tooth with severe curvature.

Methodology: Twenty standardized simulated curved root canals were prepared to an apical size of 0.25 mm using PTN and TS ($n = 10$ canal/group) nickel–titanium files. A jig was constructed to enable reproducible image acquisition using a photographic camera. Pre- and post-instrumented images were recorded and superimposed using a computer software. The ability of the instruments to remain centered in the canal was determined by calculating a centering ratio at three independent points of the simulated canal: coronal, middle and apical third of the curvature,

* Corresponding author.

E-mail: simone.staffoli@uniroma1.it (S. Staffoli).

Peer review under responsibility of Società Italiana di Endodonzia.



Production and hosting by Elsevier

<https://doi.org/10.1016/j.gien.2018.05.002>

1121-4171/© 2018 Società Italiana di Endodonzia. Production and hosting by Elsevier B.V. This is an open access article under the CC BY-NC-ND license (<http://creativecommons.org/licenses/by-nc-nd/4.0/>).

PAROLE CHIAVE

NichelTitanio;
Capacità di centratura;
Trattamento termico;
2Shape;
Protaper Next.

using a computer software. Statistical analysis was performed using one-way analysis of variance (ANOVA) followed by independent sample *t*-test at 5% significance level.

Results: No significant difference was found between the two systems ($p > 0.05$). At the apical third, the mean centering ratio was significantly higher than the centering ratio of the coronal and the middle thirds in both TS and PTN ($p < 0.05$).

Conclusions: There were no significant differences in the centering ability of the ProTaper Next and 2Shape systems in simulated severe curved canals. Both systems exhibited some degree of transportation, especially in the apical third.

© 2018 Società Italiana di Endodonzia. Production and hosting by Elsevier B.V. This is an open access article under the CC BY-NC-ND license (<http://creativecommons.org/licenses/by-nc-nd/4.0/>).

Riassunto

OBIETTIVI: L'obiettivo è confrontare la centratura di preparazione tra Protaper Next e 2Shape in canali artificiali con curvature complesse.

MATERIALI E METODI: 20 molari inferiori artificiali con canali colorati sono stati divisi random per i due tipi di strumenti testate.

Le immagini prima e dopo la strumentazione sono state rilevate mediante un software (Adobe Photoshop 7.0.1; Adobe Systems, Inc., Mountain View, California, USA). La capacità di centratura degli strumenti è stata calcolata misurando i canali in tre differenti porzioni: Coronale, Media ed Apicale.

ANOVA test è stato successivamente eseguito per determinare i valori ottenuti.

RISULTATI: Non sono risultate differenze significativamente tra la capacità di centratura di preparazione tra i due strumenti testati.

CONCLUSIONI: No differenze significative tra i due strumenti testati, entrambi hanno evidenziato un certo trasporto della centratura della preparazione soprattutto nel terzo apicale.

© 2018 Società Italiana di Endodonzia. Production and hosting by Elsevier B.V. Cet article est publié en Open Access sous licence CC BY-NC-ND (<http://creativecommons.org/licenses/by-nc-nd/4.0/>)

Introduction

The purpose of instrumentation is mechanical debridement, the creation of space for the delivery of irrigation and optimized canal geometries for adequate obturation,¹ while maintaining the original canal anatomy.² In the curved canal, large stainless-steel files (SS) are less flexible and tend to straighten and transport the canal with creating of apical zips and ledges.³ In danger zone areas, such straightening may lead to strip perforations.⁴

Nickel-titanium (NiTi) instruments have been reported to have a decreased tendency for canal transportation and better centering ability than SS⁵ due to their greater elasticity.⁶ Manufacturers strive to improve NiTi instruments by changing their design and enhancing the structural alloy in an attempt to improve their mechanical performance.^{4,7,8}

ProTaper Next (PTN; Dentsply Sirona, Ballaigues, Switzerland) is made of M-wire heat-treated alloy with an asymmetric square cross-section. The PTN system is consist of X1 (17/.04), X2 (25/.06), X3 (30/.07), X4 (40/.06), and X5 (50/.06) files. 2Shape (TS; MicroMega, Besancon, France) is made of T-wire heat-treated alloy with an asymmetric triangular cross-section. The 2S system is composed of TS1 (25/.04), TS2 (25/.06), F35 (36/.06), and F40 (40/.04) files.

To our knowledge, no research investigated the centering ability of TS instruments. Thus the purpose of the present study was to evaluate the centering ability of PTN and TS instruments in terms of maintaining the original root canal configuration in a simulated tooth with severe curvature. The null hypothesis was that there would be no significant difference between the PTN and TS in terms of shaping abilities.

Materials and methods

In order to standardize the root canal curvature, 20 artificial molar tooth models (MM tooth; Micro-Mega) that having severely MB and ML canals ($>60^\circ$)⁹ were selected. The working length (WL) of the ML and MB canals were 23.5 mm and 23 mm respectively. An apical foramen size of 0.1 mm was confirmed by a #10 K-file (Dentsply Sirona). Each simulated canal was colored with blue ink injected using a 27-G closed-end tip and side-vented needle (Ultradent Products, Inc., South Jordan, UT). The canals were randomly assigned to two groups ($n = 10$) according to the system that was used for canal instrumentation.

In Group 1, MB and ML canals were prepared using One G (Micro-Mega), 2Shape TS1 (25/.04) and TS2 (25/.06) files at 300 rpm and 1.2 Ncm torque values using VDW Gold (VDW, Munich, Germany) endodontic motor.

In Group 2, MB and ML canals were prepared using PathFile 1 and 2 (Dentsply Sirona), ProTaper X1 (17/.04) and X2 (25/.06) files at 300 rpm and 2 Ncm torque values using VDW Gold endodontic motor.

A single operator with experience in rotary systems performed all instrumentation procedures according to the manufacturer's instructions. Each new instrument was used to prepare only two canals. Between each preparation step, apical patency was confirmed by using a #10 K-file until the tip of the file could be seen protruding through the apical foramen. The canal was irrigated with 1.0 mL sterile water using a 27-gauge needle after each file and as a final rinse. Each tooth was embedded in a putty base without obscuring the canals. A jig was constructed to

enable reproducible image acquisition using a photographic camera (EOS 70D; Canon, Tokyo, Japan). Three reference points were marked around the tooth position to allow for exact superimposition of the images. Pre- and post-instrumented images were recorded. Then, the images were superimposed using a computer software (Adobe Photoshop 7.0.1; Adobe Systems, Inc., Mountain View, CA, USA). The ability of the instruments to remain centered in the canal was determined by calculating a centering ratio at three independent points (coronal, middle, and apical) of the simulated canal.

The calculation of the centering ratio was used the following formula: $(X1-X2)/Y$ ($X1$ – the maximum extent of canal movement in one direction, $X2$ – the movement in the opposite direction, Y – the wideness of the final canal preparation). The calculation was made using a computer software (ImageJ; NIH, Bethesda, MD).

Statistical analysis was performed using SPSS 22.0 (IBM-SPSS Inc., Chicago, IL, USA) using one-way analysis of variance (ANOVA) followed by independent sample *t*-test at 5% significance level.

Results

The mean centering ratio for TS and PTN were 0.42 and 0.43, respectively. No significant difference was found between the different systems ($p > 0.05$) as shown in Fig. 1. At the apical third, the mean centering ratio was significantly higher than the centering ratio of the coronal and the middle thirds in both TS and PTN ($p < 0.05$) (Fig. 2). There was no difference between the coronal third and the middle third with the different systems.

Discussion

In the past, files and reamers were manufactured from either carbon-steel or SS. The relatively high modulus of elasticity of these materials made it difficult for the larger file sizes to negotiate curved canals.¹⁰ NiTi rotary files are manufactured from a NiTi alloy that is significantly more elastic than SS¹¹ and was developed by William Buehler in 1962.¹¹ In 1988, Walia et al. introduced NiTi for the manufacturing of endodontic instruments.¹²

Since the introduction of this alloy, a number of different files have been developed from NiTi. Many studies demonstrate that NiTi instruments remain better centered in the canal compared to SS. Esposito and Cunningham¹³ compared NiTi hand and engine-driven files to SS hand files in curved canals. They found that for instruments larger than ISO size 30, both hand and rotary NiTi files were significantly more effective than SS in maintaining the original path of the canal. Glossen et al. reported similar findings with instruments larger than size 45.¹⁴

However, transportation of the canal can still occur with NiTi instruments in the apical, middle, and coronal thirds. Over the years, many NiTi instruments have been developed to improve root canal preparation. Hand and rotary instruments are available in various designs that differ in tip and taper design, rake angles, helical angles, pitch and different types of alloys.¹⁵

Numerous studies compared the ability of several new rotary NiTi systems to maintain original canal shape and therefore remain better centered.^{7,16–18} The present study focused on two relatively new rotary NiTi systems with asymmetrical cross-section and with a different type of heat treated NiTi alloy. PTN is a M-wire alloy and TS is a T-wire

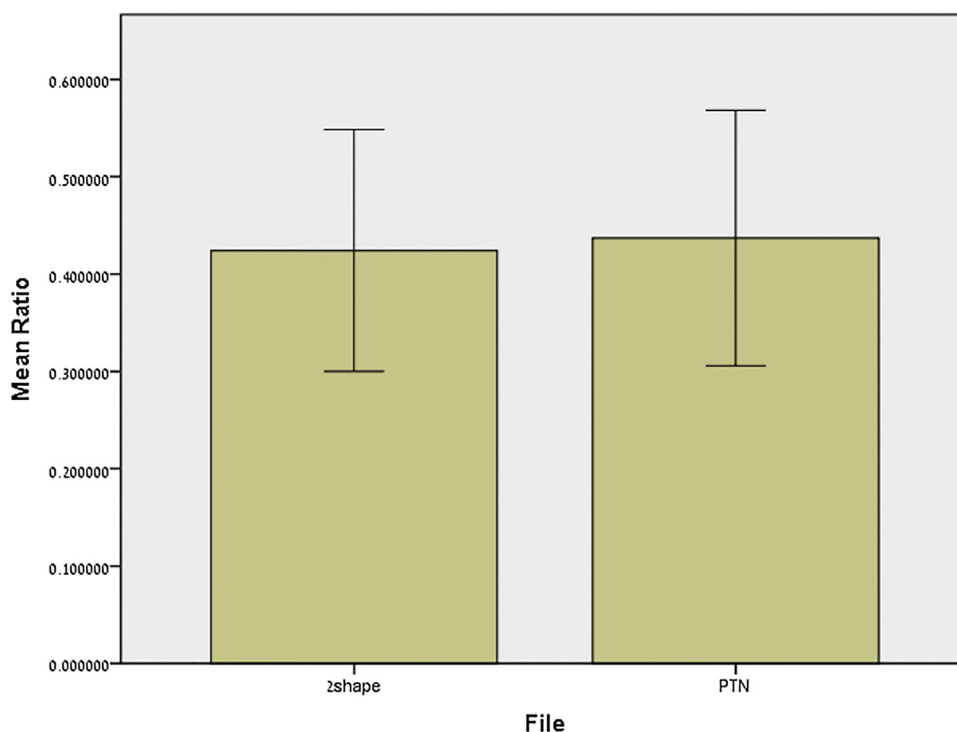


Figure 1 Total mean centering ratio of 2Shape and ProTaper Next.

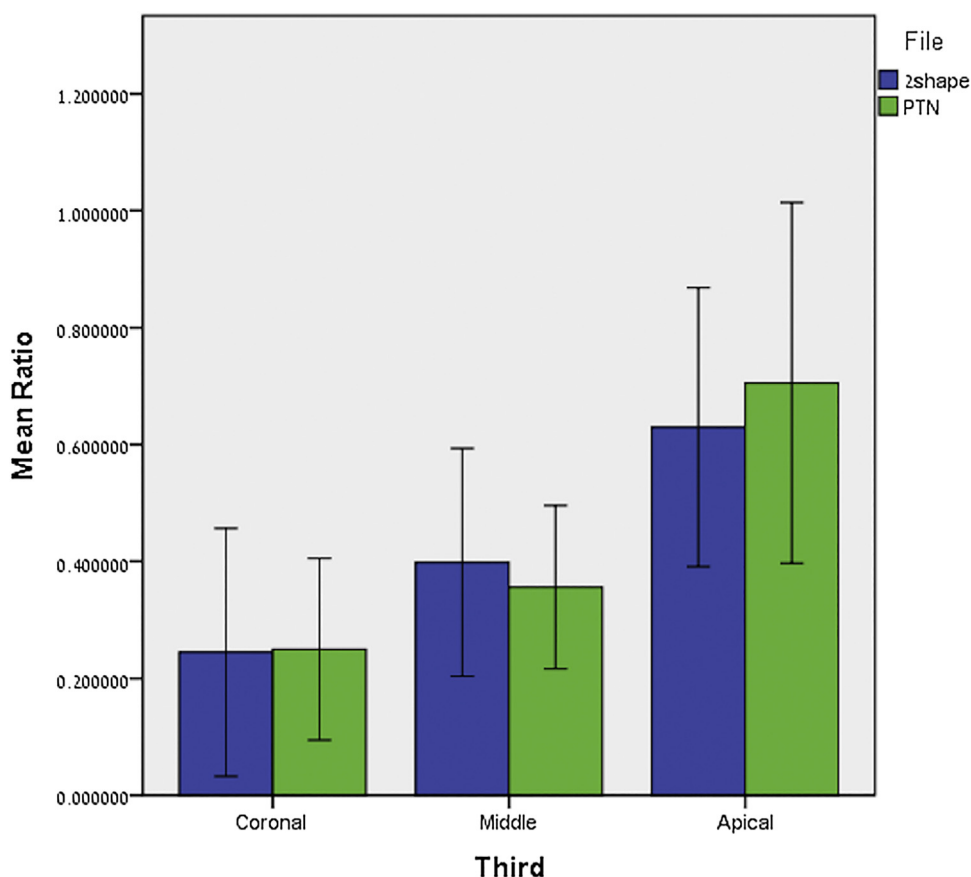


Figure 2 Mean centering ratio of 2Shape and ProTaper Next at the coronal, middle and apical third of the c.

alloy. Both M-wire and T-wire are nitinol after a proprietary thermomechanical processing procedure that increased the flexibility and the fatigue resistance.

In the present study, both PTN and TS exhibit some degree of deflection of the original canal axis. There were no significant differences between the tested file systems. Both systems showed significantly more deflection at the apical third of the simulated canal.

It would be of clinical interest to investigate the performances and centering abilities of these systems in severely curved canals in human teeth.

Conclusion

Based on the parameters examined in this study and within its limitations, it can be concluded that there were no significant differences in the centering ability of the PTN and 2Shape systems in simulated severe curved canals. Both systems exhibited some degree of transportation, especially in the apical third.

Clinical relevance

The respect of the original anatomy is one on the goals of modern endodontics.

Investigation may help the clinical expectation of the instruments tested and help clinicians.

Conflict of interest

The authors deny any conflicts of interest related to this study.

Acknowledgement

Thanks to the companies that provided the materials to make this research possible.

References

1. Peters OA. Current challenges and concepts in the preparation of root canal systems: a review. *J Endod* 2004;30:559–67.
2. Schilder H. Cleaning and shaping the root canal. *Dent Clin North Am* 1974;18:269–96.
3. Weine FS, Kelly RF, Lio PJ. The effect of preparation procedures on original canal shape and on apical foramen shape. *J Endod* 1975;1:255–62.
4. Walton RE, Torabinejad M. Principles and practice of endodontics. Elsevier Health Sciences; 2014: 210.
5. McSpadden JT. Rationales for rotary nickel-titanium instruments. Chattanooga, TN: NT Co; 1994.

6. Miura F, Mogi M, Ohura Y, Hamanaka H. The super-elastic property of the Japanese NiTi alloy wire for use in orthodontics. *Am J Orthod Dentofacial Orthop* 1986;**90**:1–10.
7. Hülsmann M, Peters OA, Dummer PM. Mechanical preparation of root canals: shaping goals, techniques and means. *Endod Top* 2005;**10**:30–76.
8. Koch K, Brave D. Real world endo: design features of rotary files and how they affect clinical performance. *Oral Health* 2002;**92**:39–49.
9. Marending M, Biel P, Attin T, Zehnder M. Comparison of two contemporary rotary systems in a pre-clinical student course setting. *Int Endo J* 2016;**49**:591–8.
10. Ponti TM, McDonald NJ, Kuttler S, Strassler HE, Dumsha TC. Canal-centering ability of two rotary file systems. *J Endod* 2002;**28**:283–6.
11. Buehler WJ, Gilfrich JV, Wiley RC. Effect of low-temperature phase changes on the mechanical properties of alloys near composition TiNi. *J Appl Phys* 1963;**34**:1475–7.
12. Walia H, Brantley WA, Gerstein H. An initial investigation of the bending and torsional properties of Nitinol root canal files. *J Endod* 1988;**14**:346–51.
13. Esposito PT, Cunningham CJ. A comparison of canal preparation with nickel-titanium and stainless steel instruments. *J Endod* 1995;**21**:173–6.
14. Glosson CR, Haller RH, Dove SB, Carlos E. A comparison of root canal preparations using Ni-Ti hand, Ni-Ti engine-driven, and K-Flex endodontic instruments. *J Endod* 1995;**21**:146–51.
15. Lim YJ, Park SJ, Kim HC, Min KS. Comparison of the centering ability of Wave One and Reciproc nickel-titanium instruments in simulated curved canals. *Restor Dent Endod* 2013;**38**:21–5.
16. Al-Sudani D, Al-Shahrani S. A comparison of the canal centering ability of ProFile, K3, and RaCe Nickel Titanium rotary systems. *J Endod* 2006;**32**:1198–201.
17. Paleker F, Van Der Vyver PJ. Comparison of canal transportation and centering ability of k-files, proglider file, and g-files: a micro-computed tomography study of curved root canals. *J Endod* 2016;**42**:1105–9.
18. Jain A, Asrani H, Singhal AC, Bhatia TK, Sharma V, Jaiswal P. Comparative evaluation of canal transportation, centering ability, and remaining dentin thickness between WaveOne and ProTaper rotary by using cone beam computed tomography: an in vitro study. *J Conserv Dent* 2016;**9**:440–4.